

# Certificate of Analysis



EHRENSTORFER™

## ISO Guide 34 Reference Material

### Product Identification

Article Code: DRE-C10662000

Article Name: Boldenone

Formula: C19H26O2

Mol. Weight: 286.41

CAS No.: 846-48-0

Lot Number: G979496

Expiry Date: 24.08.2022

Storage Temperature: 20°C ± 4°C

Storage and handling: The RM should be stored in the original sealed bottle at the temperature given above. After use the bottle should be tightly closed and protected from moisture.

Purity: 97.01% (g/g)

Expanded Uncertainty U= 0.42% (g/g)

The uncertainty of this standard is calculated in accordance with the ISO Guide 34 and EURACHEM/CITAC Guide - Quantifying Uncertainty in Analytical Measurement, Second Edition. The expanded uncertainty is  $U(\text{exp}) = u(\text{RM}) \times k$ , where  $k$  is the coverage factor at the 95% confidence level ( $k=2$ ). Uncertainty  $u(\text{RM})$  is based on the combination of the uncertainties associated with each individual operation involved in the analysis of the product:  $u(\text{RM}) = \sqrt{u(\text{char})^2 + u(\text{bb})^2 + u(\text{Its})^2 + u(\text{sts})^2}$ ;  $u(\text{char})$  is the uncertainty of characterisation;  $u(\text{bb})$  uncertainty of homogeneity test;  $u(\text{Its})$  uncertainty of stability test long-term;  $u(\text{sts})$  uncertainty of stability test short-term.  $u(\text{Its})$  and  $u(\text{sts})$  are not included in the calculation as the stability statement is based on real evidence opposed to simulation.

Minimum sample: 1 mg is recommended as the minimal sample amount. If less material is used, it is recommended to increase the certified uncertainty by a factor of two for half sample and a factor of four for a quarter of sample.

Intended use: Use this RM as calibrant for chromatography or any other analytical technique.

### Analytical Data

Traceability of chromatography: To the International System of Units (SI).

Instrument: UHPLC/DAD

Detection: DAD

Column: LUNA Omega C18 1.6 µm 100 x 2.1 mm

Inj.-Vol.: 4 µl

Flow: 0.5 ml/min

Ret.Time: 5.20 min

Method Details

Eluent A: WA + 0.5% H3PO4

Eluent B: Acetonitrile

Time[min]	Eluent A [%]	Eluent B [%]
0	90	10
0.3	90	10
8	0	100
9.5	0	100
10	90	10

### Comment

Traceability: The balances used are calibrated with weights traceable to the national standards (DKD).

Calibrated class A glassware is used for volumetric measurements.

Water Content: 0.19% (g/g) by Karl-Fischer-Titration ( $U(\text{exp}) = 0.19\%$  (g/g)).

Purity was determined by chromatographic assay, corrected by water content and/or residue solvents.

Identity: EA, NMR, RT, IR, UV, MS

Attachment: Exemplary chromatogram of given method

Certificate Revision 1 - 24.08.2018 - M. Beck

Certified on: 24.08.2018

Certified by: M. Beck

RM Release

The LGC Labor GmbH, accredited by DAkkS as indicated by the accreditation number D-RM-19883-01 & D-PL-19883-01, has shown competence based on ISO Guide 34:2009 with relevant parts of DIN EN ISO/IEC 17025:2005 for production of certified reference materials in form of organic pure substances and in form of single and multi-component solutions of organic pure substances.


LGC Labor GmbH - Bgm.-Schlosser-Straße 6A - 86199 Augsburg - Germany  
Phone +49 821 906080 - Fax +49 821 9060888 - augsburg.inquiry@lgcgroup.com  
The warranty for this product is limited to the purchasing price of this product.

Data file: 10662000-18-r001.dx  
Inj. volume [µl]: 4.0  
Acq. method: Gradient\_10-100\_P.amx

Instrument: UHPLC 2  
Sequence Name: 01122017-1a  
Injection date: 12/1/2017 10:58:12 PM  
Location: P2-D3

B

Sample Description Boldenone

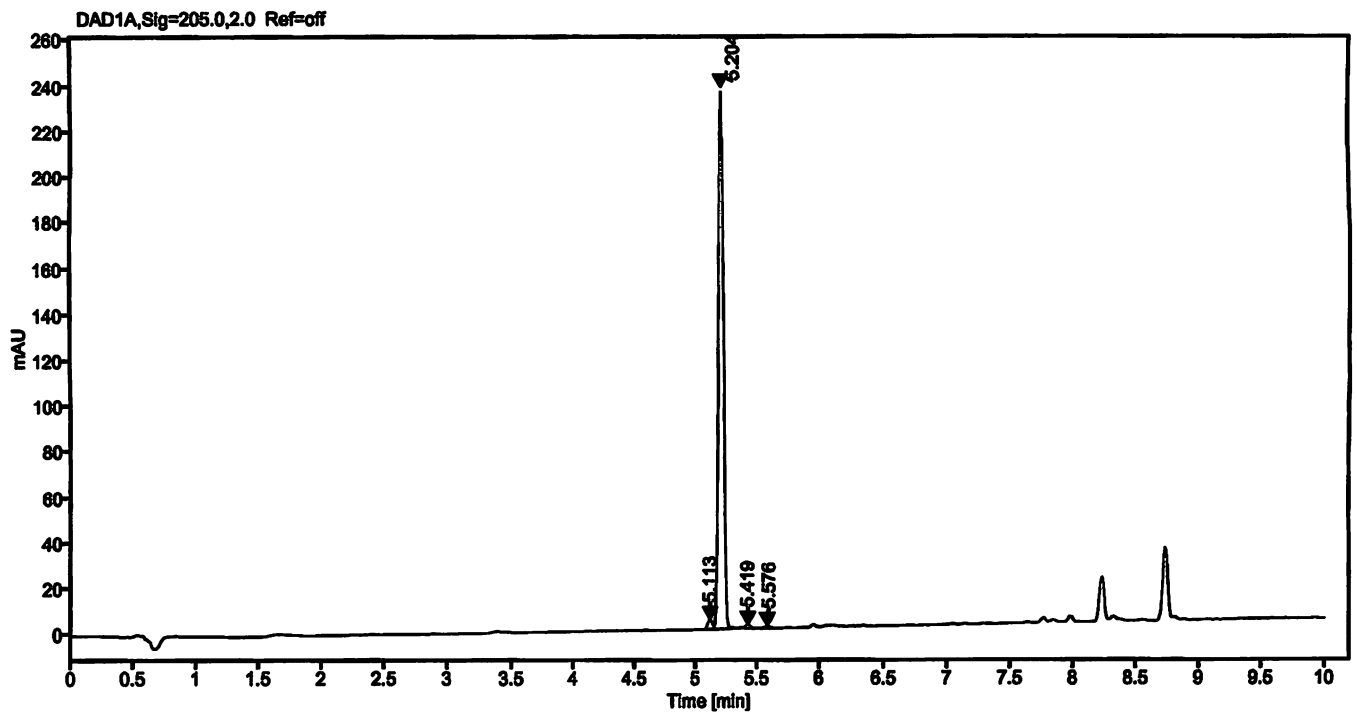

Signal: DAD1A, Sig=205.0, 2.0 Ref=off

Nr.	RT [min]	Area	Height	Area%
1	5.113	10.34376	3.90	1.54
2	5.204	654.37309	236.47	97.47
3	5.419	4.30685	1.40	0.64
4	5.576	2.32018	0.79	0.35
	Sum	671.34		

*P. Dea*